

## CMV

- Detection and quantification of Cytomegalovirus (CMV) specific DNA
- Parallel testing within Herpes- and Polyomavirus test kit panel
- Ready-to-use kit including Internal Control and Quantification Standards
- Quantification in International Units (IU)
- Compatible with various Real-Time PCR platforms
- CE-IVD marked *in-vitro* diagnostic test

### RealStar<sup>®</sup> CMV PCR Kit 1.0

Prod. No 021013

**For use with:**

ABI Prism<sup>®</sup> 7500 SDS and 7500 Fast SDS, m2000rt, Mx 3005P<sup>™</sup> QPCR System, VERSANT<sup>™</sup> kPCR Molecular System AD, LightCycler<sup>®</sup> 480 Instrument II, Rotor-Gene<sup>™</sup> 3000/6000, Rotor-Gene<sup>™</sup> Q 5/6 plex Platform

### RealStar<sup>®</sup> CMV PCR Kit 1.2

Prod. No 021212



**For use with:**

SmartCycler<sup>®</sup> II, LightCycler<sup>®</sup> 1.2 / 1.5 / 2.0

always a drop ahead.



## RealStar<sup>®</sup> CMV PCR Kit

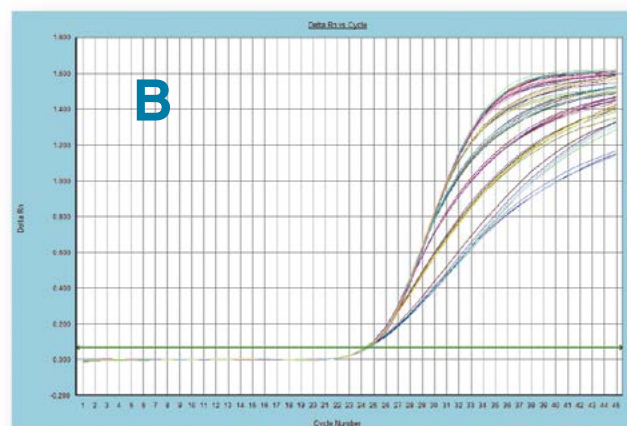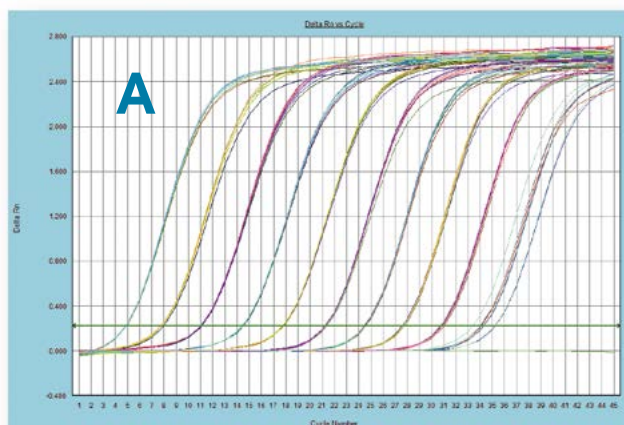

Dilution series of CMV specific DNA, ranging from  $10^0$  to  $10^9$  IU/ $\mu$ l, detected in the FAM detection channel [A]. The Internal Control is detected in the JOE detection channel [B].

