

## Chikungunya

- Detection of Chikungunya Virus specific RNA
- Parallel testing within tropical RT-PCR test kit panel
- Ready-to-use kit including Internal and Positive Control
- Compatible with various Real-Time PCR platforms
- CE-IVD marked *in-vitro* diagnostic test

### RealStar<sup>®</sup> Chikungunya RT-PCR Kit 2.0 Prod. No 012013

**For use with:**

ABI Prism<sup>®</sup> 7500 SDS and 7500 Fast SDS,  
Mx 3005P<sup>™</sup> QPCR System,  
VERSANT<sup>®</sup> kPCR Molecular System AD,  
LightCycler<sup>®</sup> 480 Instrument II,  
Rotor-Gene<sup>®</sup> 6000,  
Rotor-Gene<sup>®</sup> Q 5/6 plex Platform, CFX96<sup>™</sup> /  
CFX96<sup>™</sup> Deep Well Real-Time System



### RealStar<sup>®</sup> Chikungunya RT-PCR Kit 1.1 Prod. No 011112

**For use with:**

LightCycler<sup>®</sup> 1.2 / 1.5 / 2.0

**always a drop ahead.**

## RealStar<sup>®</sup> Chikungunya RT-PCR Kit

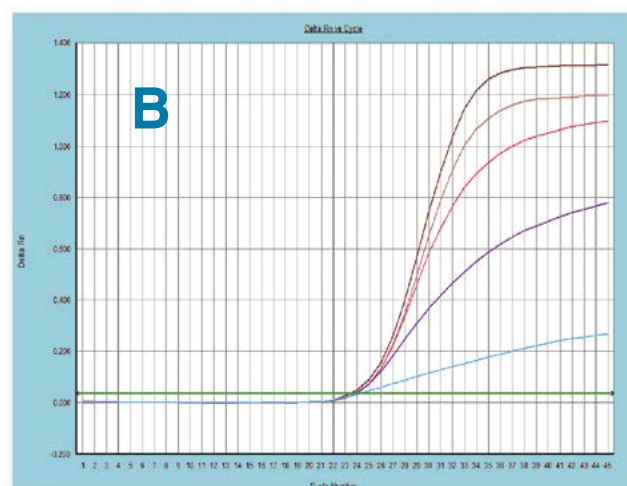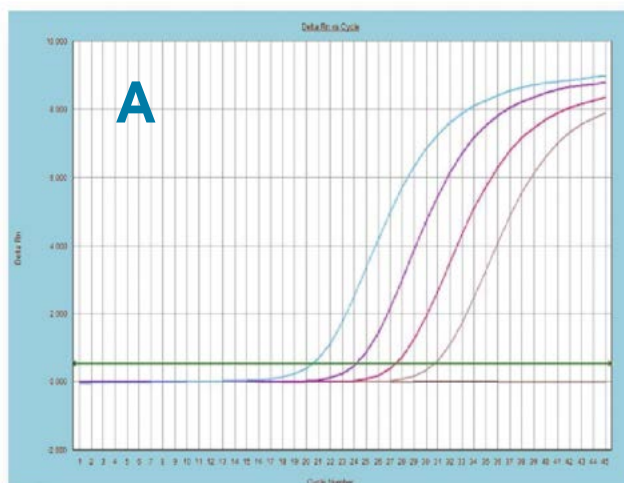

Dilution series of Chikungunya virus specific RNA, ranging from  $10^1$  to  $10^4$  copies/ $\mu$ l, detected in the FAM detection channel [A]. The Internal Control (IC) is detected in the JOE detection channel [B].

